

Display Report

Analysis Info


Analysis Name D:\data\fenglei\CS018215_GD1_01_27997.d
Method 1008-MID.m
Sample Name CS018215
Comment

Acquisition Date 4/9/2024 9:35:17 AM

Operator Demo User
Instrument impact II 1825265.10256

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	150 m/z	Set End Plate Offset	-500 V	Set Dry Gas	3.0 l/min
Scan End	8000 m/z	Set Charging Voltage	2000 V	Set Divert Valve	Source
		Set Corona	0 nA	Set APCI Heater	0 °C

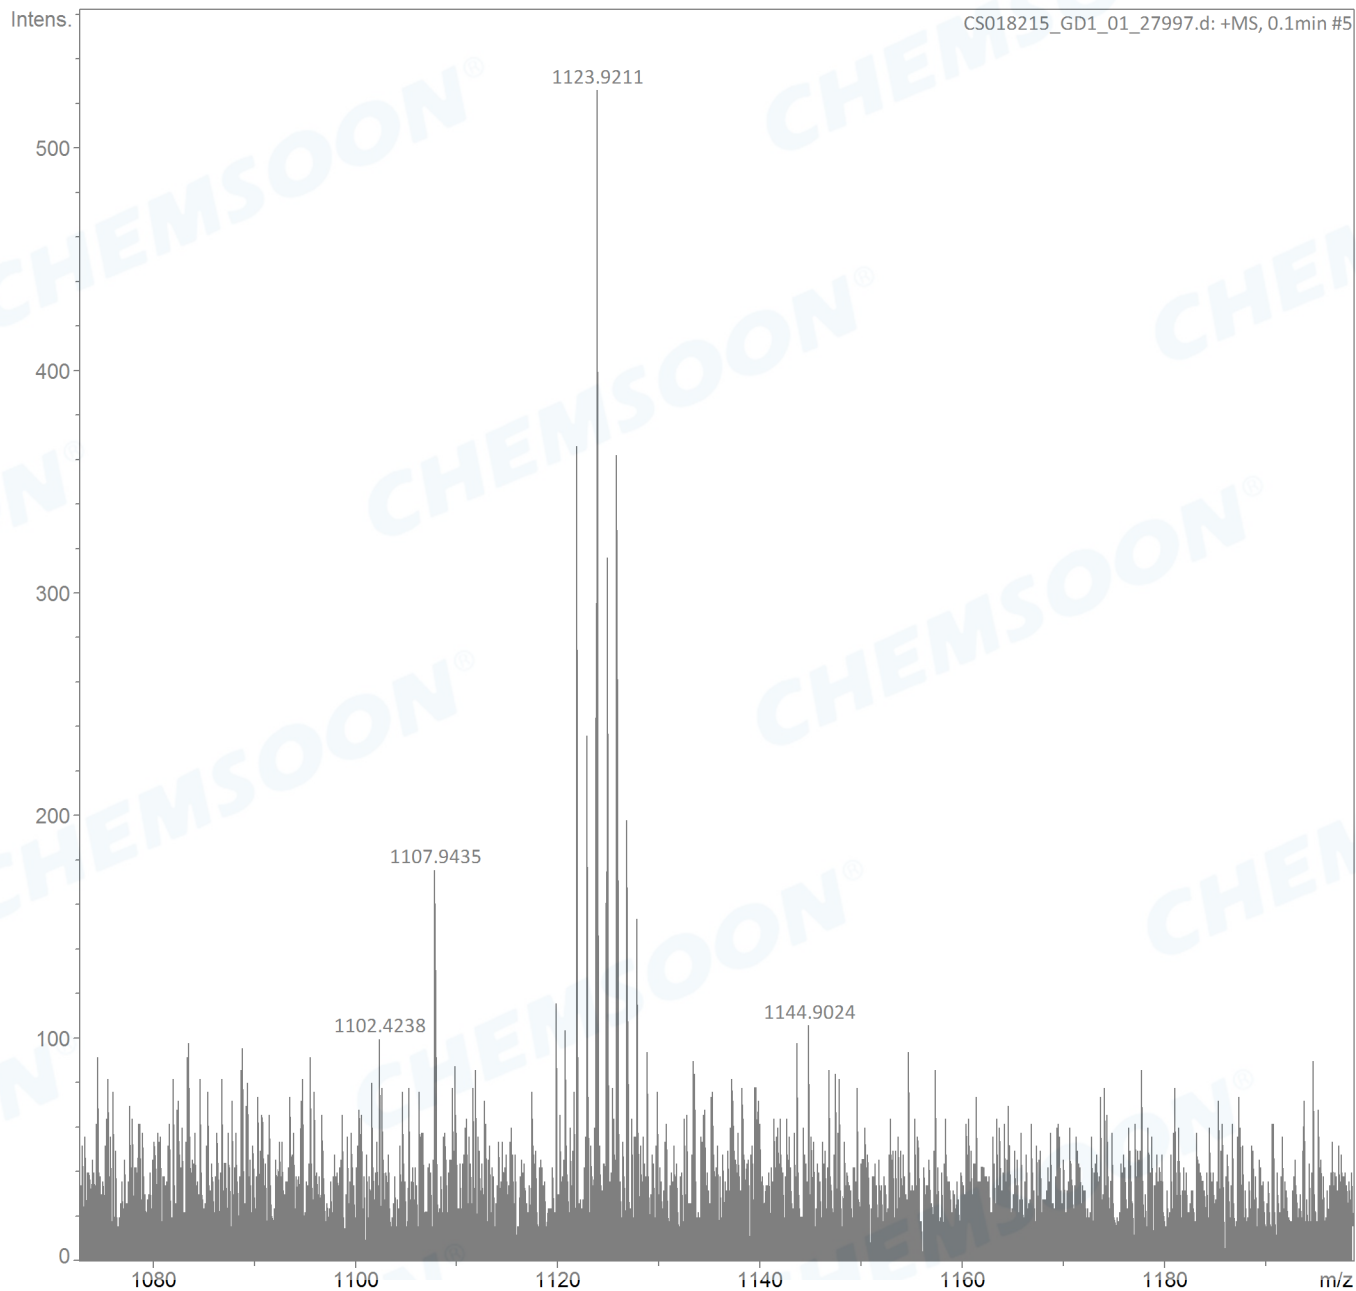

CS018215_GD1_01_27997.d

Bruker Compass DataAnalysis 4.4

printed: 4/9/2024 10:13:13 AM

by: demo

Page 1 of 1