

Display Report

Analysis Info


Analysis Name D:\data\fenglei\CS018137_BA7_01_25927.d
Method 1008-ms.m
Sample Name CS018137
Comment

Acquisition Date 1/11/2024 11:05:19 AM

Operator Demo User
Instrument impact II 1825265.10256

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	30 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	2000 m/z	Set Charging Voltage	2000 V	Set Divert Valve	Source
		Set Corona	0 nA	Set APCI Heater	0 °C

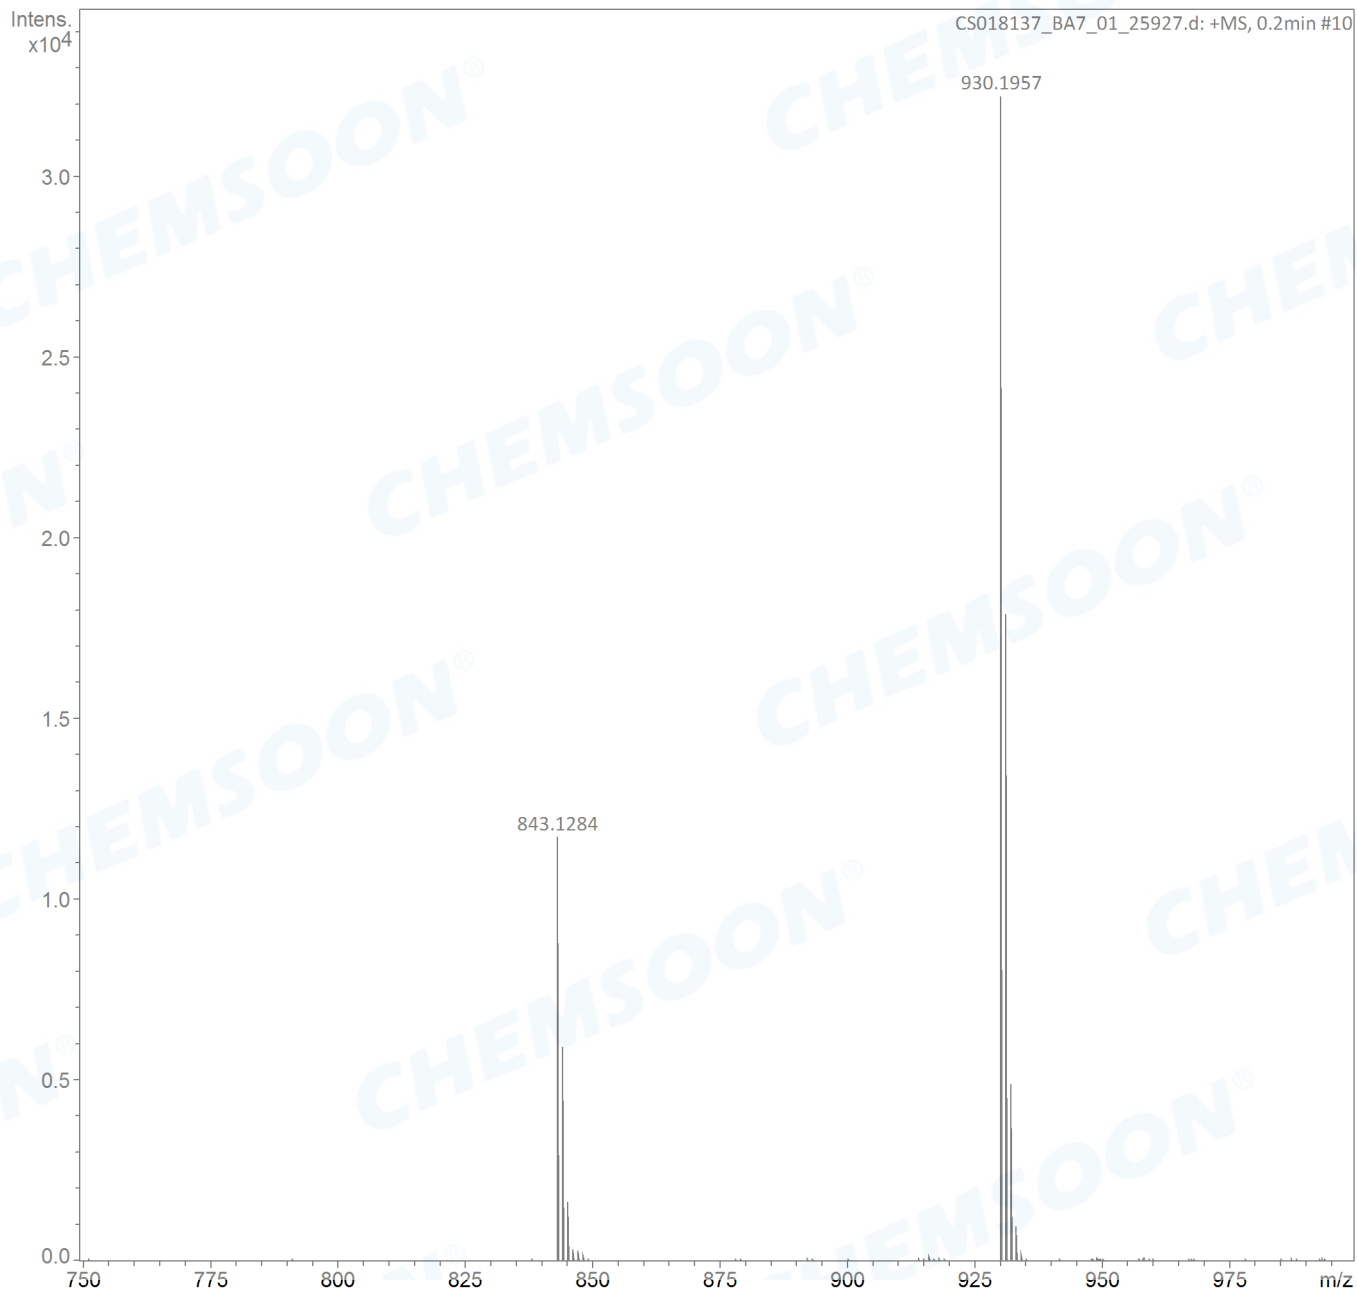

CS018137_BA7_01_25927.d

Bruker Compass DataAnalysis 4.4

printed: 1/11/2024 11:18:57 AM

by: demo

Page 1 of 1