

Display Report

Analysis Info


Analysis Name D:\data\fenglei\CS017090_RC1_01_9978.d
Method LC_TEST_001.m
Sample Name CS017090
Comment

Acquisition Date 9/13/2021 9:47:32 AM

Operator demo
Instrument impact II 1825265.10256

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	2600 V	Set Dry Heater	180 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	3000 m/z	Set Charging Voltage	2000 V	Set Divert Valve	Source
		Set Corona	0 nA	Set APCI Heater	0 °C

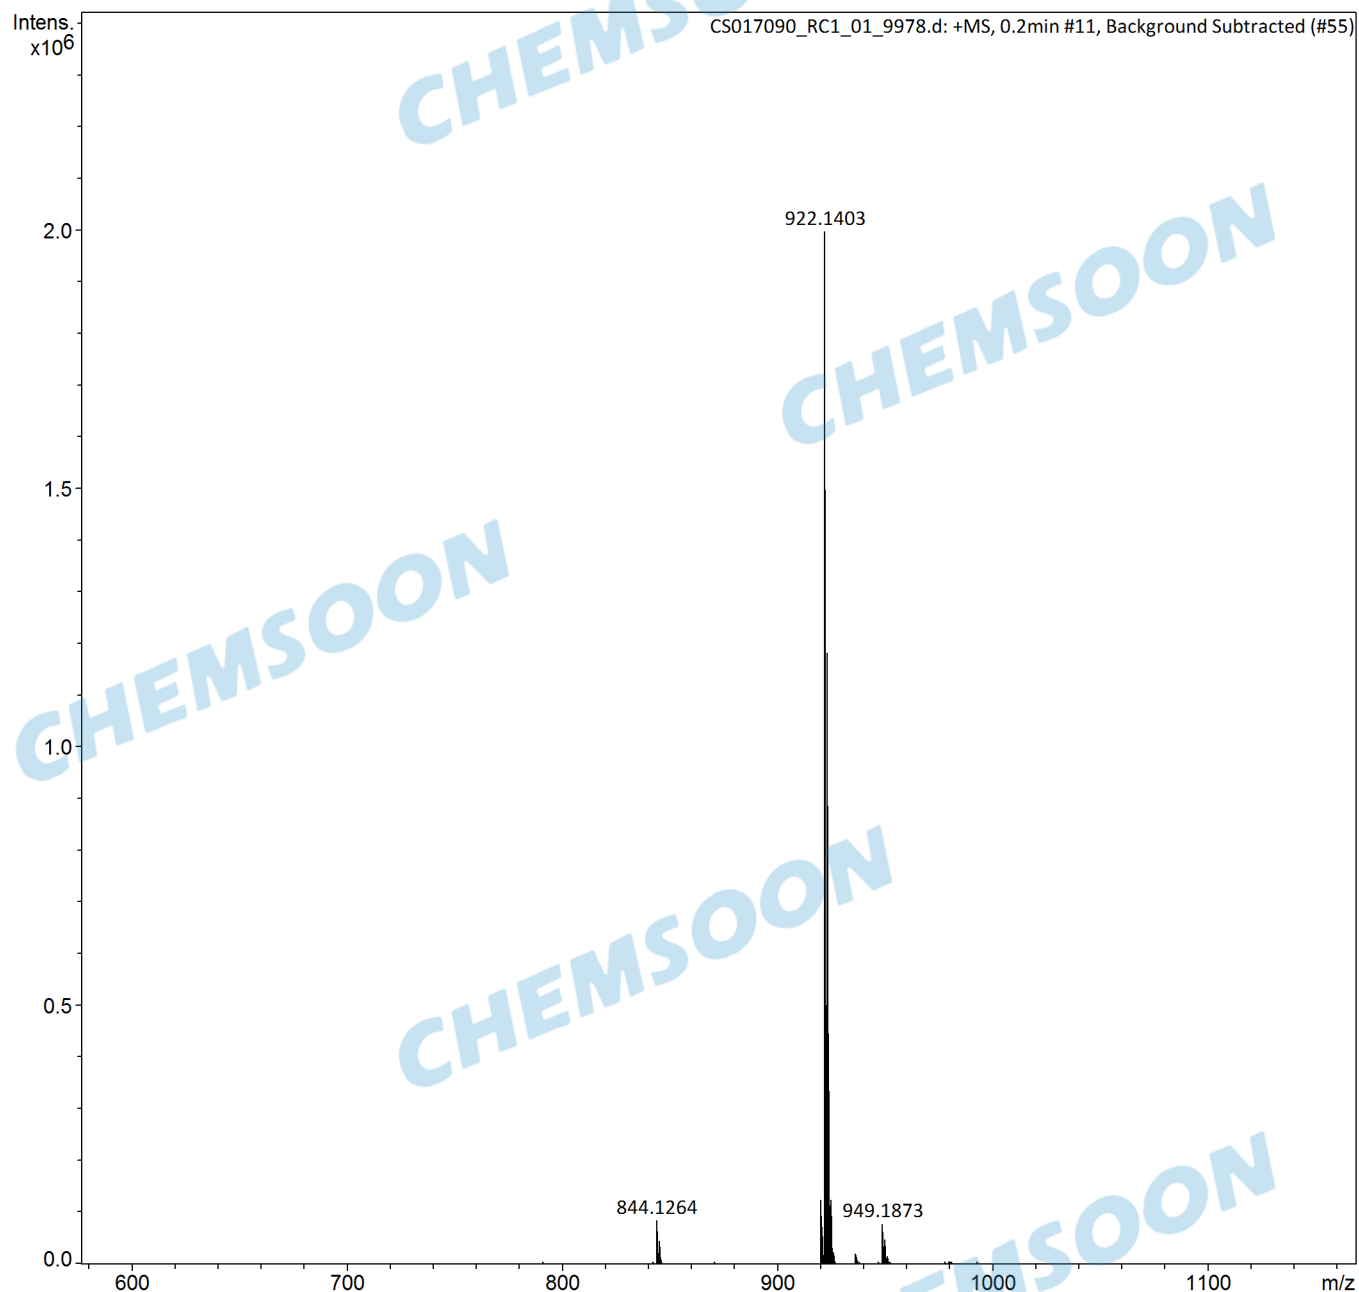

CS017090_RC1_01_9978.d

Bruker Compass DataAnalysis 4.4

printed: 9/13/2021 9:50:08 AM

by: demo

Page 1 of 1