

ANALYSIS REPORT



<Sample Information>

Sample Name : CS014123

Method Name : Normal Method(A H2O-0.1%H3PO4).1cm
Batch Name : 20191029.lcb
Location : 1-15
Inj. Volume : 1 uL
Acquisition Time : 2019/10/29 15:15:08
Modified Time : 2019/10/29 15:47:40

Level : 1
Operator : System Administrator
Modified by : System Administrator

<Chromatogram>

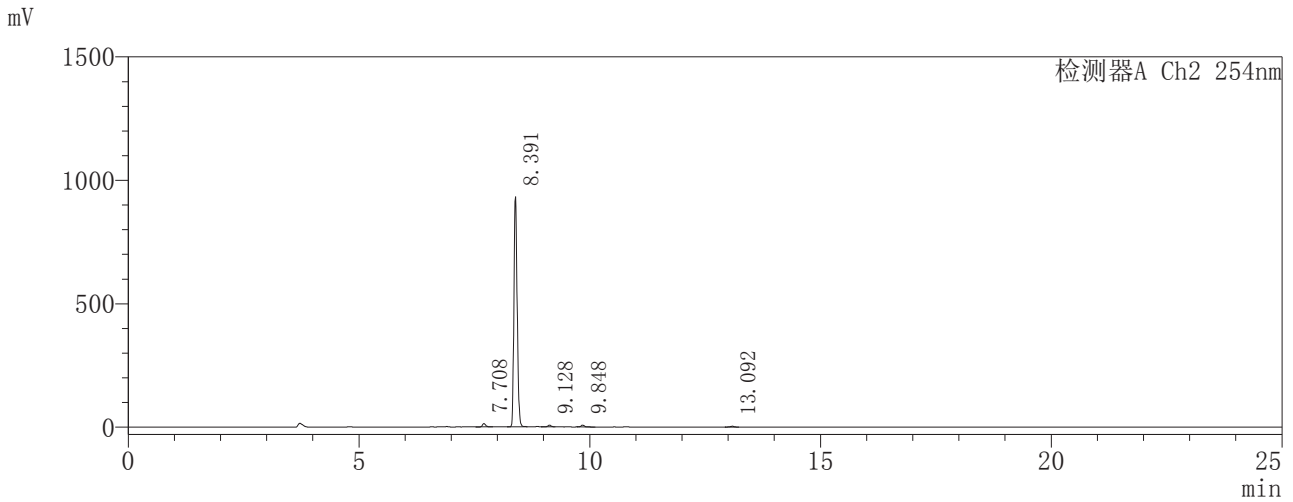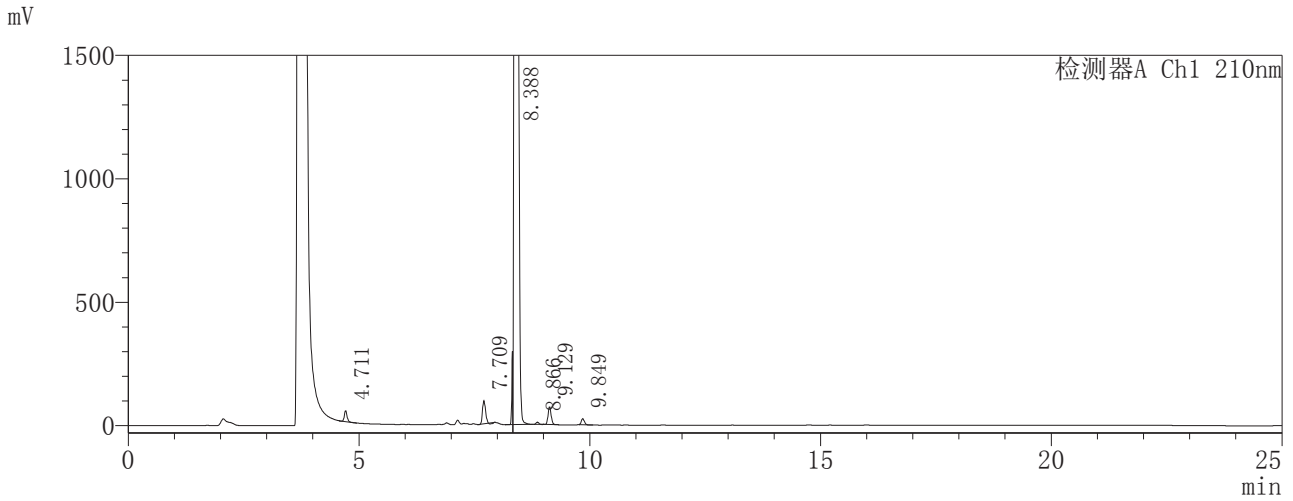

<Peak Table>

检测器A Ch1 210nm

| Number | RetTim | Area | Area% | Height |
|--------|--------|----------|---------|---------|
| 1 | 4.711 | 171052 | 0.587 | 43183 |
| 2 | 7.709 | 411166 | 1.411 | 91569 |
| 3 | 8.388 | 28058215 | 96.318 | 3995040 |
| 4 | 8.866 | 39399 | 0.135 | 8853 |
| 5 | 9.129 | 337268 | 1.158 | 71149 |
| 6 | 9.849 | 113671 | 0.390 | 24100 |
| 总计 | | 29130771 | 100.000 | 4233895 |

检测器A Ch2 254nm

| Number | RetTim | Area | Area% | Height |
|--------|--------|---------|---------|--------|
| 1 | 7.708 | 64911 | 1.377 | 13301 |
| 2 | 8.391 | 4562918 | 96.823 | 910786 |
| 3 | 9.128 | 29479 | 0.626 | 6522 |
| 4 | 9.848 | 37870 | 0.804 | 7426 |
| 5 | 13.092 | 17450 | 0.370 | 3016 |
| 总计 | | 4712627 | 100.000 | 941050 |