

ANALYSIS REPORT

<Sample Information>

Sample Name : CS015020

Method Name : Normal Method(A H2O-0.1%H3PO4).1cm

Batch Name : 20191101.lcb

Location : 1-14

Inj. Volume : 1 uL

Acquisition Time : 2019/11/1 14:25:39

Modified Time : 2019/11/1 15:06:45


Level : 1

Operator : System Administrator

Modified by : System Administrator


<Chromatogram>

mV

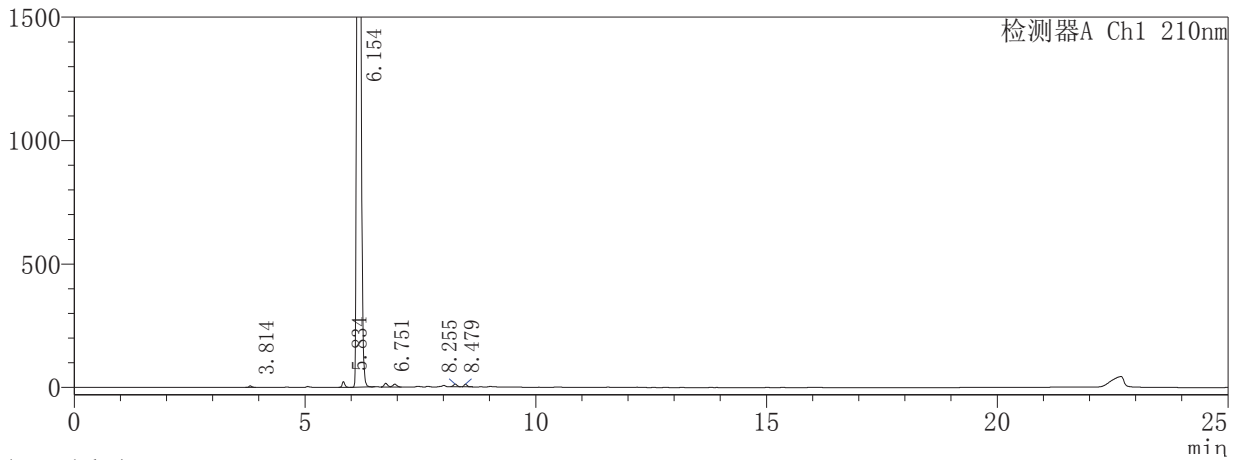

<Peak Table>

mV

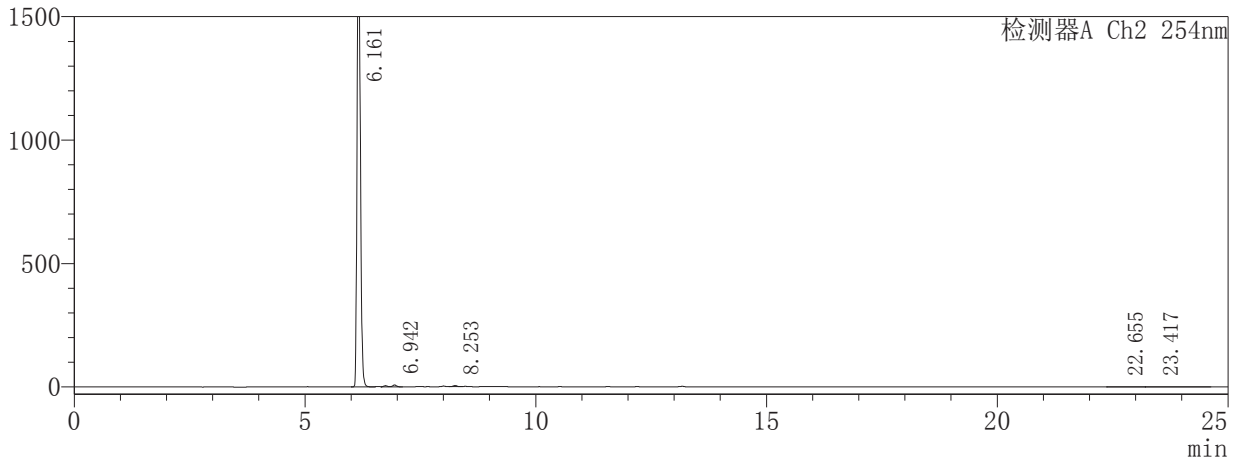

检测器A Ch1 210nm

| Number | RetTim | Area | Area% | Height |
|--------|--------|----------|---------|---------|
| 1 | 3.814 | 24540 | 0.102 | 6095 |
| 2 | 5.834 | 91216 | 0.378 | 22530 |
| 3 | 6.154 | 23759556 | 98.509 | 3998498 |
| 4 | 6.751 | 145742 | 0.604 | 14544 |
| 5 | 8.255 | 51627 | 0.214 | 9791 |
| 6 | 8.479 | 46449 | 0.193 | 10307 |
| 总计 | | 24119130 | 100.000 | 4061765 |

检测器A Ch2 254nm

| Number | RetTim | Area | Area% | Height |
|--------|--------|---------|---------|---------|
| 1 | 6.161 | 9453907 | 98.864 | 1970830 |
| 2 | 6.942 | 64297 | 0.672 | 7116 |
| 3 | 8.253 | 28276 | 0.296 | 4858 |
| 4 | 22.655 | 10288 | 0.108 | 375 |
| 5 | 23.417 | 5795 | 0.061 | 134 |
| 总计 | | 9562564 | 100.000 | 1983313 |